


PRODUCT: Information Signs  
SERIES: “X-Ray in Use”, “Darkroom in Use”, “CT in Use”, “MRI in Use”  
MODEL(S): 900X, 900D, 900CT, 900MR  
(Models with both incandescent and LED lamps–LED models have “-LED” model suffix)  
MOUNTING: Wall mount

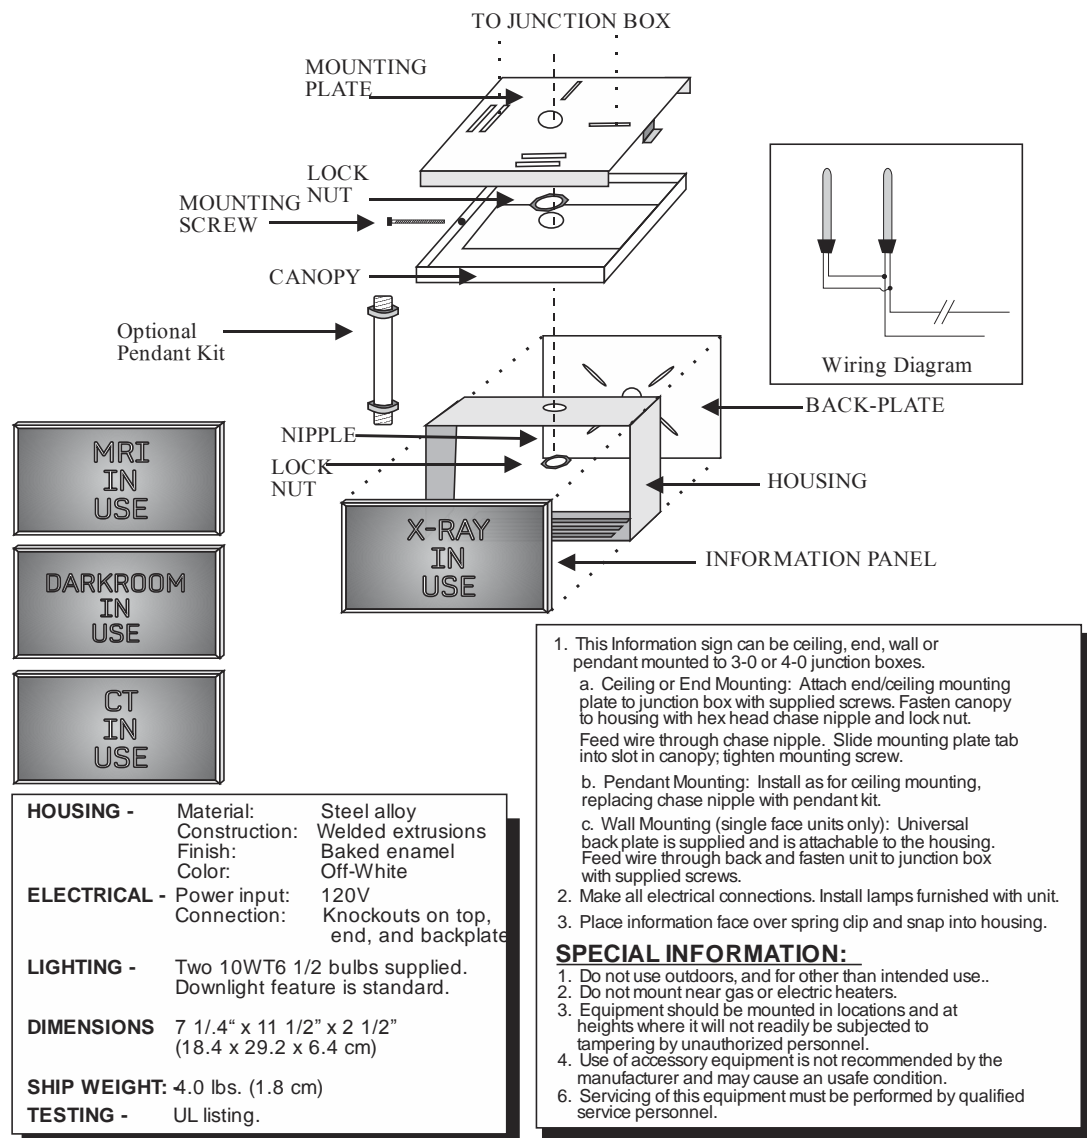

Note: LED models use two 1-Watt LED lamps – 120VAC 60Hz with 26 LED lights.